




N800起動画面



# Ga定点セル29.7646°C測定グラフ画面、測定周期2秒

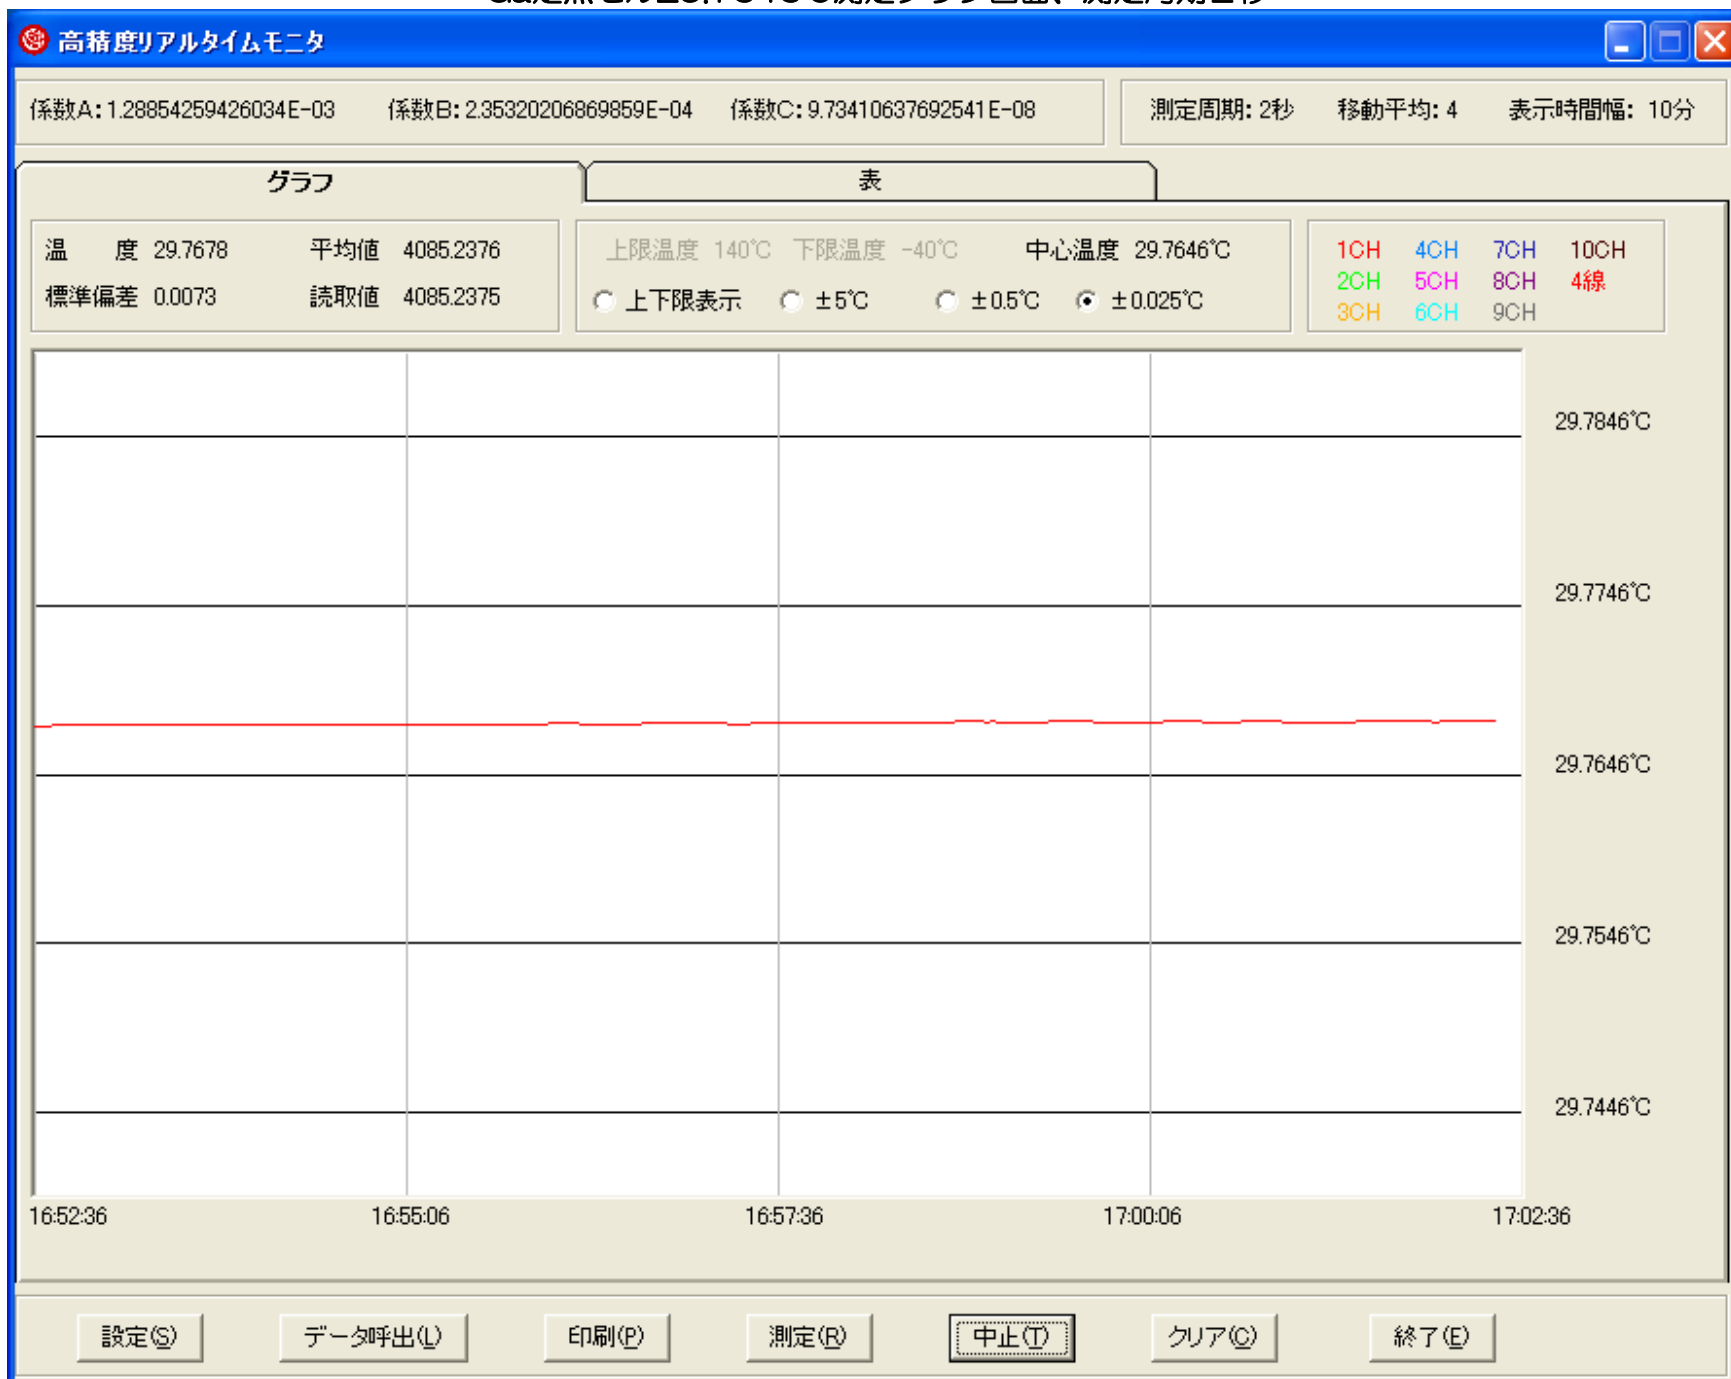

上記29.7646°C測定のカラクタ画面

高精度リアルタイムモニタ

係数A: 1.28854259426034E-03    係数B: 2.35320206869859E-04    係数C: 9.73410637692541E-08    測定周期: 2秒    移動平均: 4    表示時間幅: 10分


グラフ    表

| 時刻       | 読取值Ω      | 移動平均値Ω    | 標準偏差   | 温度°C    |
|----------|-----------|-----------|--------|---------|
| 17:01:07 | 4085.2563 | 4085.2557 | 0.0049 | 29.7677 |
| 17:01:09 | 4085.2590 | 4085.2551 | 0.0039 | 29.7677 |
| 17:01:11 | 4085.2585 | 4085.2573 | 0.0018 | 29.7677 |
| 17:01:13 | 4085.2598 | 4085.2584 | 0.0015 | 29.7677 |
| 17:01:15 | 4085.2627 | 4085.2600 | 0.0019 | 29.7677 |
| 17:01:17 | 4085.2576 | 4085.2596 | 0.0022 | 29.7677 |
| 17:01:19 | 4085.2539 | 4085.2585 | 0.0037 | 29.7677 |
| 17:01:21 | 4085.2603 | 4085.2586 | 0.0038 | 29.7677 |
| 17:01:23 | 4085.2466 | 4085.2546 | 0.0059 | 29.7677 |
| 17:01:25 | 4085.2559 | 4085.2542 | 0.0057 | 29.7677 |
| 17:01:27 | 4085.2485 | 4085.2528 | 0.0064 | 29.7677 |
| 17:01:29 | 4085.2507 | 4085.2504 | 0.0040 | 29.7678 |
| 17:01:31 | 4085.2473 | 4085.2506 | 0.0038 | 29.7678 |
| 17:01:33 | 4085.2366 | 4085.2458 | 0.0063 | 29.7678 |
| 17:01:35 | 4085.2412 | 4085.2440 | 0.0063 | 29.7678 |
| 17:01:37 | 4085.2427 | 4085.2419 | 0.0044 | 29.7678 |
| 17:01:39 | 4085.2407 | 4085.2403 | 0.0026 | 29.7678 |
| 17:01:41 | 4085.2322 | 4085.2392 | 0.0048 | 29.7678 |
| 17:01:43 | 4085.2339 | 4085.2374 | 0.0051 | 29.7678 |
| 17:01:45 | 4085.2329 | 4085.2349 | 0.0039 | 29.7678 |
| 17:01:47 | 4085.2515 | 4085.2376 | 0.0093 | 29.7678 |
| 17:01:49 | 4085.2437 | 4085.2405 | 0.0088 | 29.7678 |
| 17:01:51 | 4085.2432 | 4085.2428 | 0.0076 | 29.7678 |
| 17:01:53 | 4085.2336 | 4085.2430 | 0.0073 | 29.7678 |
| 17:01:55 | 4085.2603 | 4085.2452 | 0.0111 | 29.7678 |
| 17:01:57 | 4085.2656 | 4085.2507 | 0.0149 | 29.7678 |
| 17:01:59 | 4085.2520 | 4085.2529 | 0.0140 | 29.7677 |
| 17:02:01 | 4085.2402 | 4085.2545 | 0.0111 | 29.7677 |
| 17:02:03 | 4085.2383 | 4085.2490 | 0.0126 | 29.7678 |
| 17:02:05 | 4085.2515 | 4085.2455 | 0.0072 | 29.7678 |
| 17:02:07 | 4085.2407 | 4085.2427 | 0.0060 | 29.7678 |
| 17:02:09 | 4085.2351 | 4085.2414 | 0.0071 | 29.7678 |
| 17:02:11 | 4085.2361 | 4085.2408 | 0.0075 | 29.7678 |
| 17:02:13 | 4085.2312 | 4085.2358 | 0.0039 | 29.7678 |
| 17:02:15 | 4085.2424 | 4085.2362 | 0.0047 | 29.7678 |
| 17:02:17 | 4085.2356 | 4085.2363 | 0.0046 | 29.7678 |
| 17:02:19 | 4085.2310 | 4085.2350 | 0.0054 | 29.7678 |
| 17:02:21 | 4085.2341 | 4085.2358 | 0.0048 | 29.7678 |
| 17:02:23 | 4085.2478 | 4085.2371 | 0.0074 | 29.7678 |
| 17:02:25 | 4085.2375 | 4085.2376 | 0.0073 | 29.7678 |

設定(S)    データ呼出(L)    印刷(P)    測定(R)    中止(T)    クリア(C)    終了(E)

一般

0°C液槽内をサーミスタ温度センサ10本で測定、測定周期2秒、グラフ画面

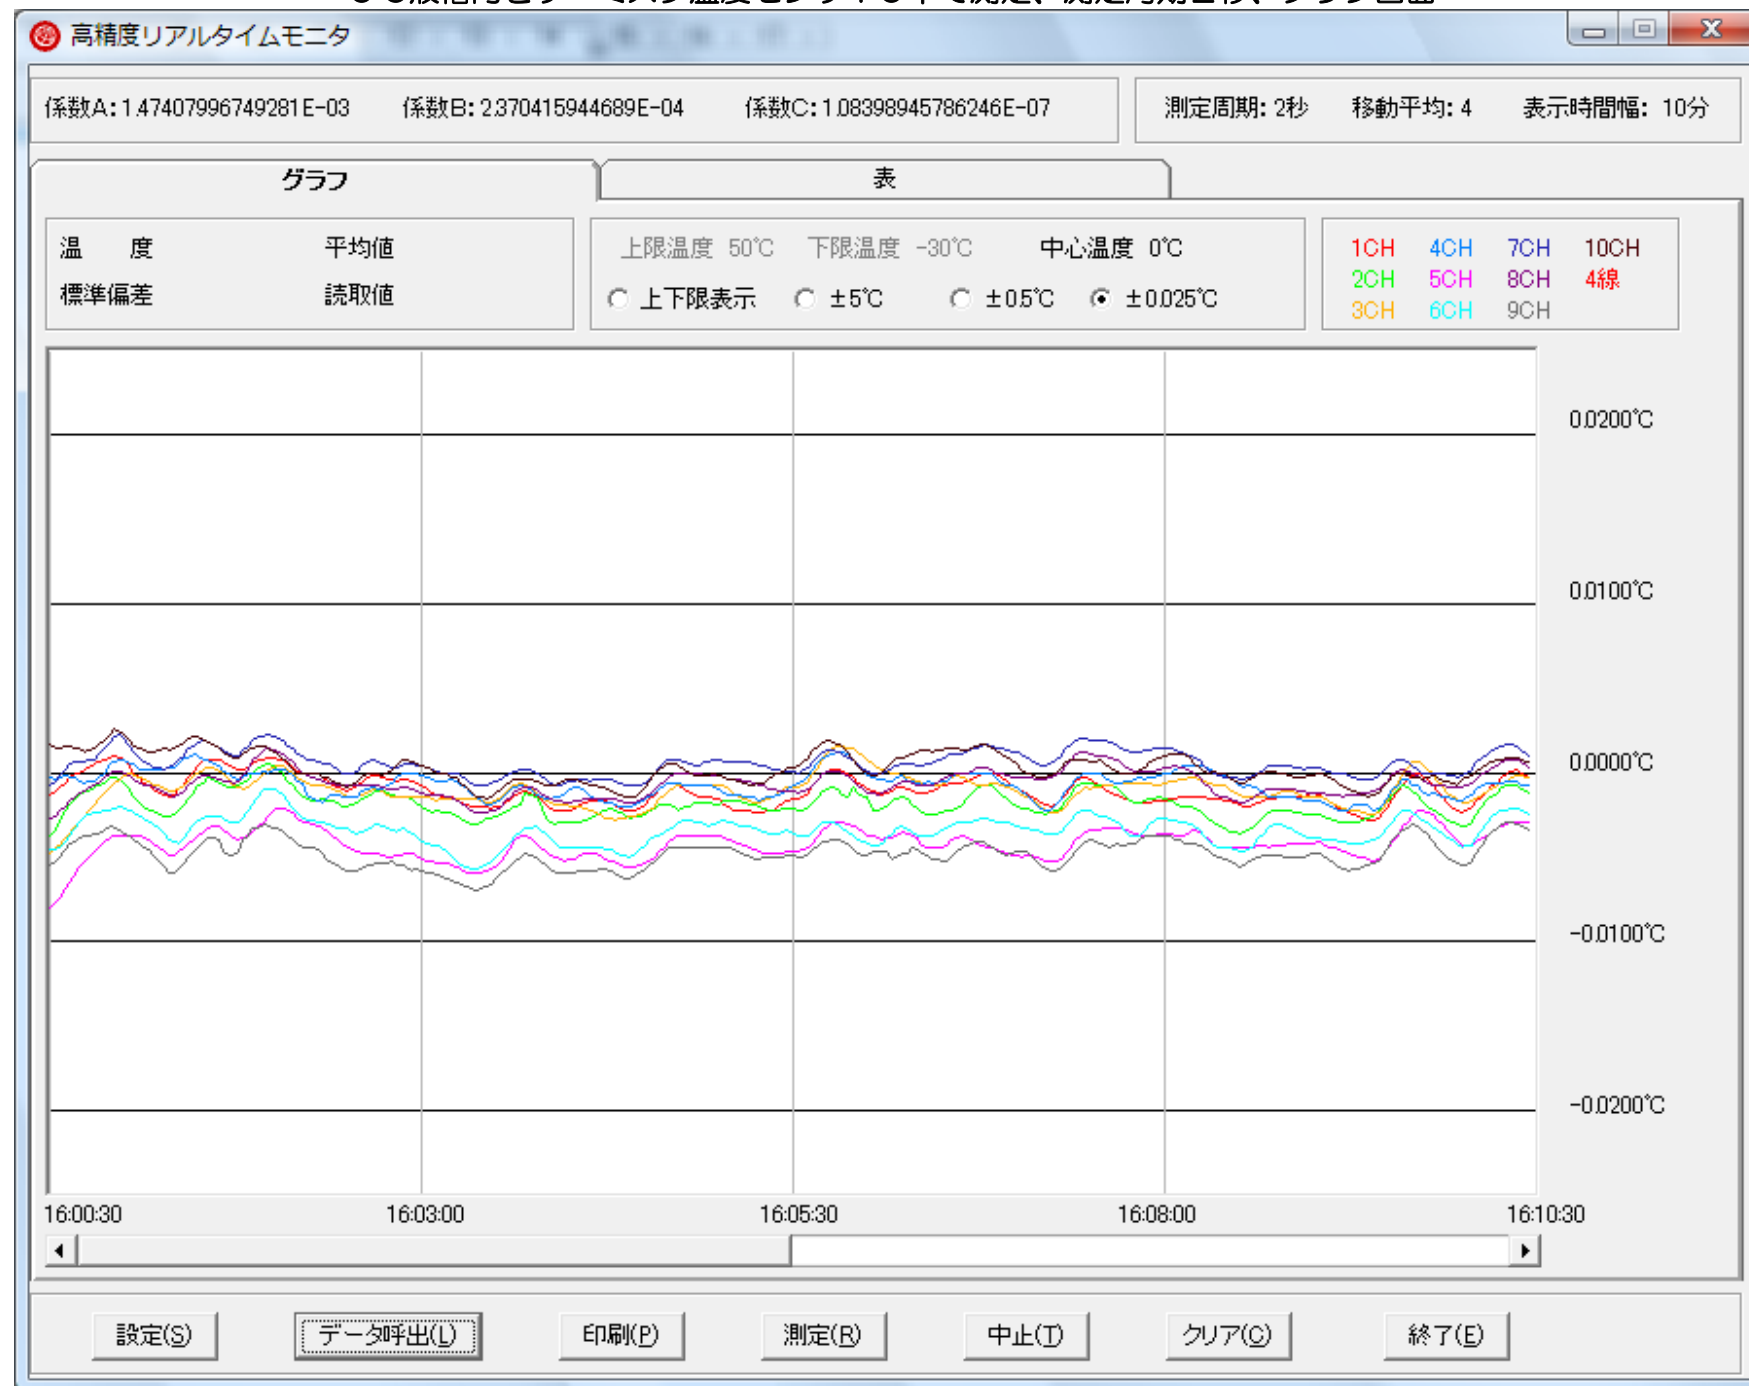

上記測定データを保存完了後データを読み出し表示、キャラクタ画面

高精度リアルタイムモニタ

係数A: 1.47407996749281E-03    係数B: 2.370415944689E-04    係数C: 1.08398945786246E-07    測定周期: 2秒    移動平均: 4    表示時間幅: 10分

グラフ    表

| 時刻       | 読取值Ω          | 移動平均値Ω        | 標準偏差      | 温度℃        | 2CH-℃      | 3CH-℃      | 4CH-℃      | 5CH-℃    |
|----------|---------------|---------------|-----------|------------|------------|------------|------------|----------|
| 16:00:30 | 94476.8515625 | 94475.7402344 | 0.9771639 | -0.0012953 | -0.0038057 | -0.0047626 | -0.0003293 | -0.00804 |
| 16:00:32 | 94475.8203125 | 94474.8457031 | 1.2266268 | -0.0011035 | -0.0033883 | -0.0045351 | -0.0004260 | -0.00770 |
| 16:00:34 | 94475.8203125 | 94473.9414063 | 1.5573679 | -0.0009096 | -0.0029086 | -0.0042667 | -0.0003118 | -0.00738 |
| 16:00:36 | 94474.4687500 | 94472.5605469 | 1.7702554 | -0.0006135 | -0.0023188 | -0.0038993 | -0.0002175 | -0.00694 |
| 16:00:38 | 94473.2734375 | 94471.3027344 | 1.7497835 | -0.0003437 | -0.0019076 | -0.0035578 | -0.0002959 | -0.00647 |
| 16:00:40 | 94472.2031250 | 94470.3183594 | 1.3283911 | -0.0001326 | -0.0015561 | -0.0032038 | -0.0003284 | -0.00605 |
| 16:00:42 | 94470.2968750 | 94469.4960938 | 0.5799696 | 0.0000437  | -0.0012609 | -0.0028961 | -0.0004661 | -0.00564 |
| 16:00:44 | 94469.4375000 | 94468.9453125 | 0.6112751 | 0.0001619  | -0.0011048 | -0.0025963 | -0.0005595 | -0.00530 |
| 16:00:46 | 94469.3359375 | 94468.2949219 | 1.1009321 | 0.0003013  | -0.0011006 | -0.0022724 | -0.0005145 | -0.00499 |
| 16:00:48 | 94468.9140625 | 94467.5175781 | 1.2129163 | 0.0004680  | -0.0009361 | -0.0019471 | -0.0004677 | -0.00468 |
| 16:00:50 | 94468.0937500 | 94466.7460938 | 0.9894154 | 0.0006335  | -0.0007591 | -0.0015952 | -0.0002905 | -0.00437 |
| 16:00:52 | 94466.8359375 | 94465.8730469 | 0.9435433 | 0.0008207  | -0.0005654 | -0.0012277 | 0.0000073  | -0.00408 |
| 16:00:54 | 94466.2265625 | 94465.4414063 | 0.7260863 | 0.0009133  | -0.0003449 | -0.0008854 | 0.0004661  | -0.00389 |
| 16:00:56 | 94465.8281250 | 94465.1875000 | 0.5034468 | 0.0009678  | -0.0003416 | -0.0006165 | 0.0005980  | -0.00378 |
| 16:00:58 | 94464.6015625 | 94465.5136719 | 1.1118549 | 0.0008978  | -0.0003687 | -0.0003551 | 0.0008153  | -0.00371 |
| 16:01:00 | 94465.1093750 | 94466.6542969 | 1.9146776 | 0.0006532  | -0.0006251 | -0.0002077 | 0.0007861  | -0.00368 |
| 16:01:02 | 94465.2109375 | 94468.0546875 | 2.3960485 | 0.0003529  | -0.0009837 | -0.0001442 | 0.0005283  | -0.00368 |
| 16:01:04 | 94467.1328125 | 94469.7343750 | 2.0709462 | -0.0000074 | -0.0014438 | -0.0001759 | 0.0004966  | -0.00370 |
| 16:01:06 | 94469.1640625 | 94471.2343750 | 1.6978128 | -0.0003291 | -0.0018266 | -0.0002515 | 0.0002459  | -0.00376 |
| 16:01:08 | 94470.7109375 | 94472.4687500 | 1.4705497 | -0.0005938 | -0.0020145 | -0.0003601 | 0.0001516  | -0.00387 |
| 16:01:10 | 94471.9296875 | 94473.5820313 | 1.3789819 | -0.0008325 | -0.0021844 | -0.0005263 | 0.0001566  | -0.00403 |
| 16:01:12 | 94473.1328125 | 94474.4648438 | 1.0626053 | -0.0010218 | -0.0022466 | -0.0006724 | 0.0001838  | -0.00424 |
| 16:01:14 | 94474.1015625 | 94475.2558594 | 0.9067522 | -0.0011915 | -0.0024653 | -0.0008449 | 0.0002388  | -0.00449 |
| 16:01:16 | 94475.1640625 | 94475.8437500 | 0.6285382 | -0.0013175 | -0.0025776 | -0.0010140 | 0.0002284  | -0.00472 |
| 16:01:18 | 94475.4609375 | 94475.9960938 | 0.4601865 | -0.0013502 | -0.0025880 | -0.0011146 | 0.0002588  | -0.00486 |
| 16:01:20 | 94476.2968750 | 94475.6621094 | 1.0651654 | -0.0012786 | -0.0025066 | -0.0011426 | 0.0003185  | -0.00486 |
| 16:01:22 | 94476.4531250 | 94474.5664063 | 2.0204289 | -0.0010436 | -0.0022445 | -0.0010390 | 0.0005454  | -0.00473 |
| 16:01:24 | 94475.7734375 | 94472.8671875 | 2.6612621 | -0.0006792 | -0.0019393 | -0.0008198 | 0.0008541  | -0.00450 |
| 16:01:26 | 94474.1250000 | 94470.9218750 | 2.6726592 | -0.0002620 | -0.0016145 | -0.0005392 | 0.0009100  | -0.00422 |
| 16:01:28 | 94471.9140625 | 94469.2363281 | 2.0273136 | 0.0000994  | -0.0011703 | -0.0002415 | 0.0010589  | -0.00398 |
| 16:01:30 | 94469.6562500 | 94467.7929688 | 1.4617311 | 0.0004090  | -0.0008117 | -0.0000114 | 0.0009542  | -0.00375 |
| 16:01:32 | 94467.9921875 | 94466.6679688 | 1.2685874 | 0.0006503  | -0.0005541 | 0.0001652  | 0.0008073  | -0.00349 |
| 16:01:34 | 94467.3828125 | 94466.1582031 | 0.9212210 | 0.0007596  | -0.0003487 | 0.0002587  | 0.0007673  | -0.00330 |
| 16:01:36 | 94466.1406250 | 94466.0273438 | 0.6998622 | 0.0007877  | -0.0004063 | 0.0002688  | 0.0005379  | -0.00317 |
| 16:01:38 | 94465.1562500 | 94466.3183594 | 0.9573288 | 0.0007252  | -0.0005683 | 0.0001305  | 0.0003577  | -0.00321 |
| 16:01:40 | 94465.9531250 | 94467.0136719 | 0.8340095 | 0.0005761  | -0.0007232 | -0.0001058 | 0.0001249  | -0.00343 |
| 16:01:42 | 94466.8593750 | 94467.6992188 | 0.7979083 | 0.0004291  | -0.0008781 | -0.0004240 | -0.0001399 | -0.00364 |
| 16:01:44 | 94467.3046875 | 94468.3457031 | 0.9276693 | 0.0002904  | -0.0008676 | -0.0007659 | -0.0003034 | -0.00387 |
| 16:01:46 | 94467.9375000 | 94468.8046875 | 0.6550398 | 0.0001920  | -0.0008201 | -0.0009421 | -0.0003681 | -0.00397 |

設定(S)    データ呼出(L)    印刷(P)    測定(R)    中止(T)    クリア(C)    終了(E)